



The Open Dentistry Journal

Content list available at: <https://opendentistryjournal.com>



RESEARCH ARTICLE

Effect of Adhesive Gap Setting on Fracture Resistance of All-ceramic Crowns

Mohammed Zahran^{1,*}

¹Department of Oral and Maxillofacial Prosthodontics, King Abdulaziz University, Faculty of Dentistry, Jeddah, Saudi Arabia

Abstract:

Background:

Several factors might affect the fracture resistance of all-ceramic crowns, including cement thickness.

Aim:

To evaluate the influence of cement thickness on the fracture resistance.

Objective:

To determine the effect of varying the adhesive gap thickness on the fracture loads of all-ceramic CEREC 3D molar crowns.

Methods:

Standardized prepared epoxy resin molar dies (Viade Inc.) were fabricated. A standard molar crown was designed using a CEREC 3D machine (Sirona Dental Systems). Twenty-four crowns were milled from Vita Mark II blocks (Vita Zahnfabrik), using adhesive gap settings of 30, 60 and 90 μm ($n=8$). A dual-cure resin cement (PanaviaF 2.0, Kuraray) was used to cement the crowns to their respective dies, following manufacturer's recommendation. After 1 week of storage in distilled water at 37°C, each crown was loaded in compression until complete failure in a universal testing machine (Instron 8501) and fracture loads (N) were recorded. Fractured specimens were sectioned to determine cement thickness. Sections were examined using a traveling light microscope to measure cement thickness. Data were statistically analyzed using one-way ANOVA test and Pearson's correlation at ($\alpha=0.05$).

Results:

The mean fracture loads and standard deviation values in N were 1,267.57 (122.82), 1,225.20 (179.46) and 1,180.76 (161.77) for the crowns with 30, 60 and 90 μm , respectively. ANOVA indicated no significant differences among mean fracture strength values ($p = 0.55$). All crowns failed in a catastrophic mode and were not repairable.

Conclusions:

Adhesive cement gap as achieved with three CEREC 3D settings from 30 to 90 μm had no significant effect on fracture strength of crowns made from Vita Mark II blocks.

Keywords: Crowns, Ceramics, Resin cements, Fracture resistance, Cement thickness, CEREC 3D.

Article History

Received: June 04, 2020

Revised: September 30, 2020

Accepted: October 13, 2020

1. INTRODUCTION

The growing demand for esthetics in combination with health and environmental concerns about some metallic restorations stimulated the profession to explore and consider metal-free tooth-colored alternatives. However, all-ceramic restorations are subject to fracture during function especially in

the posterior area. Several factors might influence the fracture resistance of all-ceramic crowns *in-vivo*. These factors can be divided into the following: factors related to the restoration (restoration geometry and thickness, material composition, processing, finishing and polishing and internal adaptation of the restoration), [1 - 6] factors related to the supporting structure (modulus of elasticity, and preparation shape, dimensions and geometry) [7 - 10], and factors related to the cementation (cement thickness, mechanical properties of the cement, adhesion mechanism and efficacy of the bond of the

* Address correspondence to this author at the Department of Oral and Maxillofacial Prosthodontics, King Abdulaziz University, Faculty of Dentistry, Jeddah, Saudi Arabia; E-mail: mzahran@kau.edu.sa

cement) [10 - 12]. Effect of cement thickness on fracture strength of ceramic restorations was studied on bilayer specimens and on restorations with real dimensions [12 - 17]. The methodology and results of these studies are summarized in (Table 1).

Till the introduction of Computer-aided Designing/Computer-aided Manufacturing (CAD/CAM) technology, the only options available for controlling the cement thickness were controlling the thickness of the die spacer paint, either by controlling the number of application or using materials with low film thickness [18], or controlling the thickness of the foil layer/s which are used for the production of porcelain jacket crowns [12]. Unfortunately, both methods are neither accurate nor precise. Currently, most CAD/CAM systems give the option to control the adhesive gap setting which is hypothesized to affect the cement thickness.

The objective of the present study was to compare the fracture load values of all-ceramic crowns made using three adhesive gap settings utilizing CAD/CAM CEREC-3D technology. The null hypothesis of this *in-vitro* study was that there is no significant difference in the fracture strength among the feldspathic crowns made with three different adhesive gap settings.

2. MATERIALS AND METHODS

The Sample size was calculated using G*power software (version 3.1) at ($\alpha=0.05$, $\beta=0.1$, Effect size =0.8) yielding a total sample size equal to 24 [19]. The effect size was calculated using the fracture load data reported previously for monolithic all-ceramic crowns fabricated with similar dimensions from the same material [20].

Twenty-four prepared replicas for 1st mandibular molar were fabricated using a highly-filled epoxy resin (Viade Products Inc. Camarillo, CA, USA), which has an elastic modulus comparable to that of human dentin and responded to 34% phosphoric acid etching with a formation of surface microroughness [21]. The epoxy replicas were duplicated from a master ivory 1st mandibular molar die that was prepared to receive all-ceramic crown with 1.5 mm occlusal reduction, 1 mm minimum axial reduction, 6 to 8° total occlusal convergence, 1 mm wide circumferential shoulder, two planes facial and lingual reduction and smooth line angles. A digital caliper (Mitutoyo Corporation, Tokyo, Japan) was used to verify that the buccolingual and mesiodistal dimensions of the replicas. These measurements showed a low variability of about 10 to 20 μm [20].

The replicas were positioned in a typodont with mesial and distal ivory teeth. Then, CEREC 3 intraoral camera was used to acquire an optical impression for the prepared replica and adjacent teeth using with a thin layer of titanium oxide as an

optical reflective medium (Vita Zahnfabrik). Twenty-four monolithic crowns were designed following the correlation mode (to correlate the designed crown's anatomy to an artificial unprepared mandibular molar) using the CEREC software (Version 2.40 R1800; Sirona Dental Systems GmbH, Bensheim, Germany). The unprepared artificial tooth was adjusted in the central fossa to receive a 3 mm loading ball.

All crowns were made using the CEREC 3 milling unit (serial number 02527) from feldspathic blocks (Vita Mark II, shade A 3.5 on Vitapan classic, 14 mm long; Vita Zahnfabrik). The crowns were milled using 1.6 mm cylindrical and cone-shaped diamonds. Cutting diamonds were changed after milling eight crowns followed by the milling unit was calibrated. The crowns were divided equally into 3 groups (n=8) using 3 adhesive gap settings (30, 60 and 90 μm). The following milling parameters were used: a spacer setting of 20 μm , margin thickness of 0 μm , and minimum thickness occlusal of 1,500 μm . After milling, Akzent glazing kit (Vita Zahnfabrik) was used to glaze all crowns according to the manufacturer's instructions.

All crowns thicknesses at the central fossae were measured to verify the minimal occlusal measurement of 1.5 mm using a calliper (Buffalo Dental Manufacturing Co., Syosset, NY, USA). A digital caliper (Mitutoyo Corporation) was used to measure the mesiodistal and buccolingual dimensions at the height of contour. Independent t-test did not reveal any statistically significant difference among the measured dimension for the 3 experimental groups [20].

The intaglio surfaces of crowns were etched with 9.6% hydrofluoric acid gel (Pulpdent Corporation, Watertown, MA, USA) according to manufacturer's recommendation. The etched surface was sprayed with water, cleaned in ultrasonic water bath for 60 seconds. The prepared surfaces of teeth replicas were treated using 40% phosphoric acid etching gel (Kuraray America Inc., New York, NY, USA) for 60 seconds, rinsed using water spray and dried with compressed oil-free air. A bonding/silane coupling agent (Clearfil SE bond/Porcelain Bond Activator, Kuraray America Inc.) was applied to the intaglio surface of the crowns following the manufacturer's instructions. A dual-cure resin cement (Panavia F 2, Kuraray America Inc.) was used to cement the crowns to their respected prepared replicas following the manufacturer's recommendation. The crowns were firstly seated using finger pressure, followed by removal of excess cement and application of air sealing gel (Oxyguard, Kuraray America Inc.) margins of the crowns for 3 minutes. Next, a static load of 22 N was applied to the crowns for 5 minutes [22]. Then, each crown surface was light-cured (Optilux 501, Kerr Demetron, Danbury, CT, USA) for 20 seconds. One hour after cementation, all crowns were stored in distilled water at 37 °C for 1 week. Tables 1 and 2 lists the materials used and some of their physical properties.

Table 1. Studies that evaluated the effect of the cement thickness on the fracture load of bilayer or crown specimens

Author (Year)	Samples	Ceramic Material	Cement Thickness	Supporting Structure	Conclusion
Scherrer (1994) [13]	Bilayer specimens	Machinable glass ceramic (2 mm in thickness)	Ranging between 26 to 297 microns	Chemical-cured composite	A gradual decrease of the fracture load was noticed, that became statistically significant at a cement thickness of 300 microns or more.
Tuntiprawon (1995) [12]	Maxillary central incisor Porcelain jacket crowns	Feldspathic porcelain	Ranging between 73 to 122 μm	Cobalt-chromium metal die	Increasing the cement thickness resulted in reduced the fracture load of the crowns.
Prakki (2007) [14]	Bilayer specimens	Feldspathic ceramic (1 or 2 mm in thickness)	100, 200 and 300 μm	Bovine dentin	For 1 mm ceramic thickness: Higher cement film thickness resulted in increased fracture load. 2 mm ceramic thickness: cement thickness has no effect.
May (2012)	Non anatomical Crowns	Feldspathic ceramic	50, 100, 300 and 500 μm	A woven glass-filled epoxy resin	Gradual reduction in the fracture load with the increase in thickness and
Rojpaibool (2017) [15]	Bilayer specimens	Lithium Disilicate ceramic (1 mm in thickness)	100 and 300 μm	Enamel or dentin	Increasing cement thickness resulted in reduction of the fracture load
Sagsoz and Yanikoglu (2018) [17]	Maxillary premolar machinable crowns	Resin nanoceramic, feldspathic glass ceramic, lithium disilicate, and leucite-reinforced ceramics	30, 90, and 150 μm	Epoxy resin replicas	Cement thickness has no effect on the fracture load

Table 2. Physical properties of materials used in the study

Material	Elastic Modulus (GPa)	Coefficient of Thermal Expansion ($10^{-6} \cdot \text{K}^{-1}$)	Flexure Strength (MPa)	Fracture Toughness ($\text{MPa} \cdot \text{m}^{1/2}$)
Vita Mark II (Vita Zahnfabrik)	70.6 ^a	8.6 ^b	103 ^c	1.26 ^d
Panavia F 2.0 (Kuraray America Inc.)	9.6 ^e	-	79 ^e	-
Epoxy resin die material (Viade Products Inc.)	12.9 ^f	-	-	-

a) Data from Trindade *et al.* [44]

b) Data from Charlton *et al.* [45]

c) Data from Bindl *et al.* [46]

d) Data from Thompson *et al.* [47]

e) Manufacturer's data

f) Neiva *et al.* [21]

The dimension from the occlusal surface of the crown to the apical surface of the replica before and after cementation was measured for each sample using a digital calliper (Mitutoyo Corporation) to ensure the crown seating [20]. A threshold of 50 μm was set for the differences between the 2 measurements. None of the samples were rejected for this reason.

All cemented samples were mounted in resin material block (SR Ivolen, Ivoclar Vivadent, Schaan, Liechtenstein) with dimensions matching the loading jig attachment. Each crown was uniaxially-loaded with a 3-mm diameter stainless steel ball at the central fossa in a universal testing machine (Instron 8501, Instron, Canton, MA, USA). Loading was conducted at cross head speed of 1 mm/minute in distilled water at room temperature. The load-displacement data were imported to a software program (Microsoft Office Excel,

Redmond, WA, USA) and load-displacement curves were generated. Load-displacement curves were analyzed, and the first drop in the curve was identified and the corresponding load (N) was recorded as load at failure.

All crowns were sectioned mesiodistally at the central fossa. Then, the cement layer thickness was measured using a travelling microscope (Mitutoyo Corporation) at three occlusal points (at the middle and near the two occluso-axial line angles). These measurements were averaged for each crown. Two samples of each group were selected for Scanning Electron Microscopy (SEM) examination. The sections from these samples were sputter-coated with 7 nm of platinum in Polaron E5100 coating unit (Polaron Equipment Ltd., Bedford, UK) and examined using SEM (Hitachi S-2500, Hitachi, Mito City, Japan).

The data was analyzed using a Statistical Package for the

Social Sciences (SPSS, Version 23, SPSS Inc., IBM, Somers, New York, USA). Both fracture load and cement thickness data were normally distributed; thus parametric tests were selected. The mean fracture loads and cement thickness were compared among the groups using one-way analysis of variance (ANOVA), followed by post-hoc Tukey’s test (when appropriate). The association between the fracture load and cement thickness was assessed using Pearson’s correlation. All statistical tests performed at a significant level of 0.05 and were two-tailed.

3. RESULTS

Mean fracture loads and standard deviations values in N were 1267.57 (± 122.82), 1225.20 (± 179.46) and 1180.76

(± 161.77) for the crowns with 30, 60 and 90 μ m adhesive gap setting, respectively (Fig. 1). One-way ANOVA revealed no statistically significant difference between the mean fracture loads of the 3 groups ($P = 0.551$). The mean cement thickness and standard deviation values in μ m were 260.9 (± 39.6), 276.4 (± 28.4) and 322 (± 31.1) for the crowns with 30, 60 and 90 μ m adhesive gap setting, respectively (Fig. 2). One-way ANOVA revealed a statistically significant difference between the mean cement thickness of the 3 groups ($P = 0.004$). Post-hoc Tukey’s test showed significantly higher cement thickness for the group with 90 μ m adhesive gap setting in comparison to the other 2 groups. Pearson’s correlation revealed no statistically significant correlation between fracture load and the cement thickness ($r = -0.357$, $P = 0.086$).

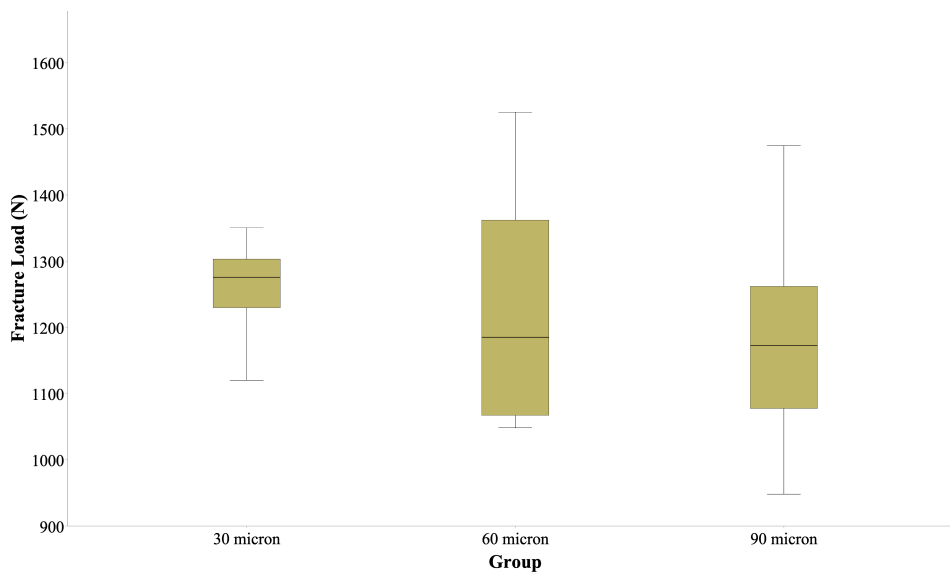


Fig. (1). Box plot graph showing the fracture load (N) for different groups based on the adhesive gap setting.

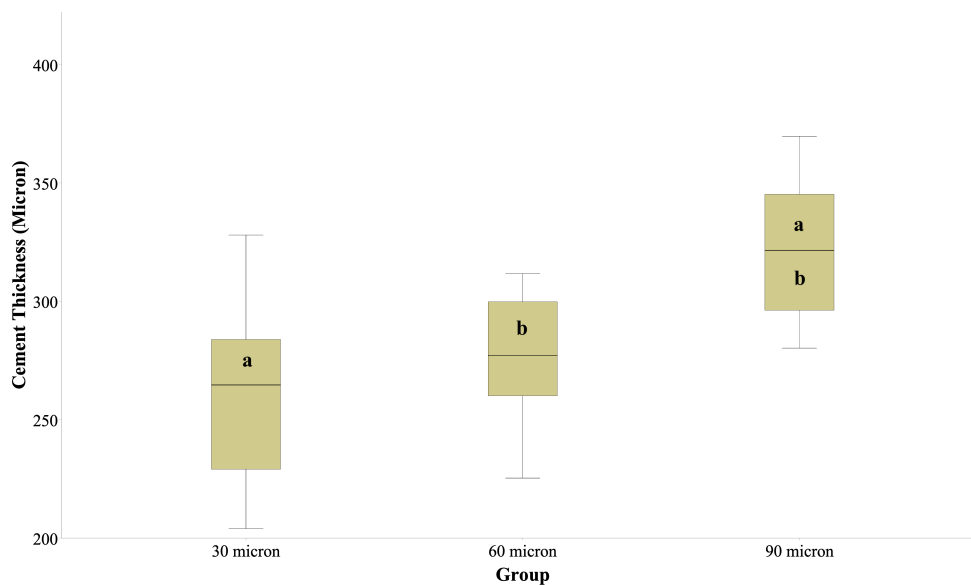


Fig. (2). Box plot graph showing cement thickness (micron) for different groups based on the adhesive gap setting (similar letters indicate statistically significant difference between the groups).

All crowns failed catastrophically and were not repairable. All fractures were confined to the ceramic material and none of them progressed to the die material. Visual examination revealed that failure originated in the contact area as a cone crack and propagated within the ceramic material till it reached the cement layer (Fig. 3). All the samples showed delamination of part of the crown at the cement interface with the other part still attached to the die material. Some large voids were noticed in the cement layer occlusally (Fig. 4). SEM images showed a homogenous ceramic structure with voids within the cement layer and adequate adaptation of the cement at the interfaces with the die and ceramic materials. Measuring the cement thickness from the SEM images revealed non-uniform thickness with higher thicknesses at the occlusal surface in comparison to the axial surfaces (Fig. 5).

4. DISCUSSION

This study failed to prove the alternative hypothesis and accepted the null hypothesis that there is no statistically significant difference between the mean fracture load values for the groups with different adhesive gap settings.

The present study followed the recommendations described by Kelly to achieve a clinically-relevant *in-vitro* load-to-failure test for all-ceramic restorations, including using a die material with elastic modulus matching the dentin, preparing the teeth according to clinical guidelines, using crowns with clinically-relevant dimensions and using a reliable, commonly-used luting cement [23]. Epoxy dies were used to avoid the variability that can be encountered with natural teeth.



Fig. (3). Microscopic image (2.5x magnification) showing cone crack (arrow) starting at the loading area which propagates till cement layer.

The use of 3-mm stainless-steel ball in the present study is expected to increase the contact pressure within the crowns compared to the clinical contact pressure. Several factors might influence the contact pressure, including the radius of the loading ball and the ratio of the elastic moduli of the dental porcelain and the loading ball [24]. Alternative approach would

be to use a tin sheet as a stress breaker between the load applicator and crown, a loading ball with a lower modulus of elasticity or a stainless-steel loading stylus with its end machined to a curvature corresponding to 40-50 mm diameter to induce clinically relevant contact pressure [23]. The contact pressure employed in this study, however, should not affect the comparison between the groups since all groups were treated equally. It has to be emphasized that the fracture load data reported in the current study should not be considered as "absolute" values and extrapolating these *in-vitro* data to the clinical performance must be considered cautiously and within the limitation of the study [25].

The fracture strength of Vita Mark II molar crowns was reported previously in the literature with a reported range between 600 and 3000 N [5, 26 - 28]. The mean fracture load of Vita Mark II crowns in the present study ranged between 1182 and 1267 N, which falls within the previously reported range. As expected for monolithic all-ceramic crowns, all Vita Mark II crowns fractured catastrophically, involving the whole crown thickness [29].

The effect of the cement thickness on fracture resistance was evaluated in several studies as shown in Table 1. These studies differ in terms of the tested materials and methodology. Four of these studies reported a significant negative relationship between the cement thickness and fracture resistance, while one study reported a positive relationship and one study reported no significant association between the two variables. It has to be emphasized that the cement thickness ranges and measurement location varied between the studies. Generally, the studies which reported a significant negative relationship used wide range of thicknesses from 100µm or below to 300µm or above. Reduction in fracture resistance was noticed for the samples with cement thicknesses larger than 300µm. Similar to the present study, Sagsoz and Yanikoglu [17] reported no difference in the mean fracture load for crowns made with different adhesive gap settings ranging between 30 and 150 µm without measuring the actual cement thickness.



Fig. (4). Microscopic image (2.5x magnification) showing voids (arrow) within the cement layer.

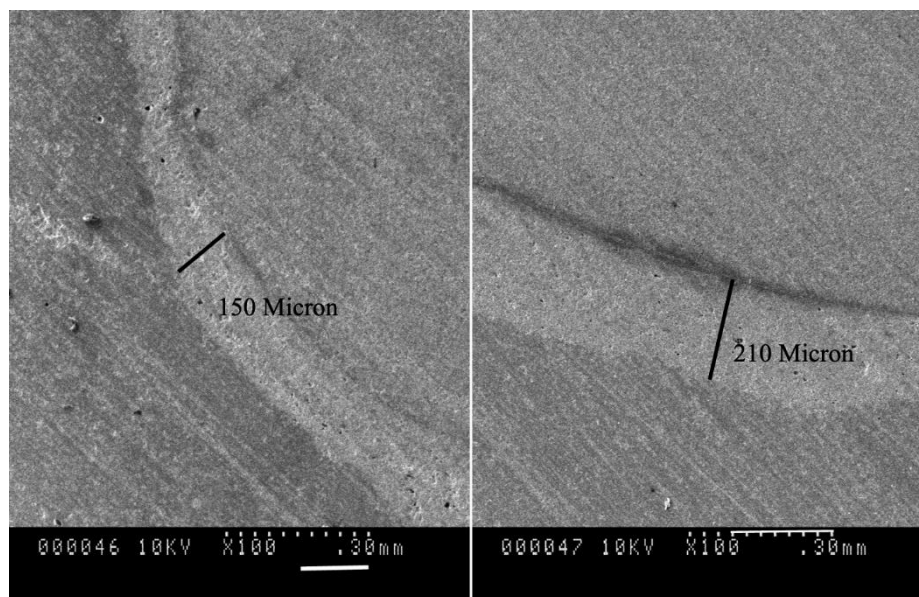


Fig. (5). SEM image showing the non-uniform distribution of the cement thickness at the axial surface (left) and occlusally (right).

It is apparent that the cement thickness is guided by the available gap between the crown and the prepared abutment. Several factors have been identified to affect the internal adaptation of the machinable all-ceramic crowns, including the angle of convergence, luting adhesive gap, luting cement composition and physical properties, occlusal anatomy, margin design and the scanning device technology [30 - 39]. It is obvious from the result of the present study that the adhesive gap setting does not reflect the actual cement thickness. This can be attributed to the acquisition and milling unit limitations. The cement thickness for the 60 μ m group falls within the previously reported by Zeltner *et al.* in which bluecam was used to scan preparation and crowns were milled using similar setting used in the current study [36]. Other studies reported lower mean thickness using bluecam and omincam with adhesive gap setting of 60, 70 and 80 μ m [32, 33, 40]. This can be attributed to the improvements in acquisition and milling devices. It worth mentioning that comparing the results of the present study to previous studies should be done with caution due to the differences in the methodology and acquisition and milling devices used. Interestingly, a recent systematic review revealed no significant effect of the impression technique (conventional versus digital) on the internal adaptation of full-coverage fixed restorations [41].

Rekow *et al.* [42] conducted factorial analysis of some variables influencing stresses in all-ceramic crowns using finite element analysis. They studied the effect of seven factors (crown material, crown thickness, cuspal inclination, cement elastic modulus, cement thickness, supporting tooth core, and location of occlusal loading). 80 and 100 μ m cement thicknesses were used. Cement modulus of elasticity and thickness accounted for only 5.5% and 1.4% of the variability in the principal stresses in the crown, respectively. These findings are in agreement with the present study. The higher mean cement thickness reported for different groups in the present study, which ranges between 260 and 322 μ m, is not expected to

change principal stresses within the crowns significantly. It seems that achieving cement thickness below 100 μ m occlusally is a challenging task. Pilo and Cardash evaluated the cement thickness under metal-ceramic crowns cemented using zinc phosphate cement to extracted teeth due to periodontal issues and reported occlusal cement thickness of 310 μ m [43]. Zeltner *et al.* [36] compared the internal adaptation of machined crowns using the digital workflow to crowns made using conventional workflow and heat-press technique as a control and found better internal adaptation for the control group compared to machined crowns, with mean occlusal internal gap for the machined crowns around 200 μ m and 89 μ m for the control group.

CONCLUSION

Within the limitations of this *in vitro* study, the following conclusions can be drawn:

- There is no statistically significant effect of using different adhesive gap settings (30, 60 and 90 μ m) on the fracture strength of all-ceramic crowns.
- Varying the cement thickness (200 - 360 μ m) does not affect the fracture strength significantly.
- The adhesive gap setting does not reflect the actual cement thickness for the milled crown.

ETHICS APPROVAL AND CONSENT TO PARTICIPATE

Not applicable.

HUMAN AND ANIMAL RIGHTS

Not applicable.

CONSENT FOR PUBLICATION

Not applicable.

AVAILABILITY OF DATA AND MATERIALS

Not applicable.

FUNDING

None.

CONFLICT OF INTEREST

The authors declare no conflict of interest, financial or otherwise.

ACKNOWLEDGEMENTS

Declared none.

REFERENCES

- [1] Deany IL. Recent advances in ceramics for dentistry. *Crit Rev Oral Biol Med* 1996; 7(2): 134-43. [http://dx.doi.org/10.1177/10454411960070020201] [PMID: 8875028]
- [2] Morena R, Lockwood PE, Fairhurst CW. Fracture toughness of commercial dental porcelains. *Dent Mater* 1986; 2(2): 58-62. [http://dx.doi.org/10.1016/S0109-5641(86)80052-5] [PMID: 3458634]
- [3] Kon M, Kawano F, Asaoka K, Matsumoto N. Effect of leucite crystals on the strength of glassy porcelain. *Dent Mater J* 1994; 13(2): 138-47. [http://dx.doi.org/10.4012/dmj.13.138] [PMID: 7758273]
- [4] Albakry M, Guazzato M, Swain MV. Effect of sandblasting, grinding, polishing and glazing on the flexural strength of two pressable all-ceramic dental materials. *J Dent* 2004; 32(2): 91-9. [http://dx.doi.org/10.1016/j.jdent.2003.08.006] [PMID: 14749080]
- [5] Chen HY, Hickel R, Setcos JC, Kunzelmann KH. Effects of surface finish and fatigue testing on the fracture strength of CAD-CAM and pressed-ceramic crowns. *J Prosthet Dent* 1999; 82(4): 468-75. [http://dx.doi.org/10.1016/S0022-3913(99)70036-3] [PMID: 10512968]
- [6] Hojjatie B, Anusavice KJ. Three-dimensional finite element analysis of glass-ceramic dental crowns. *J Biomech* 1990; 23(11): 1157-66. [http://dx.doi.org/10.1016/0021-9290(90)90008-Q] [PMID: 2277050]
- [7] Doyle MG, Munoz CA, Goodacre CJ, Friedlander LD, Moore BK. The effect of tooth preparation design on the breaking strength of Dicor crowns: 2. *Int J Prosthodont* 1990; 3(3): 241-8. [PMID: 2083010]
- [8] Doyle MG, Goodacre CJ, Munoz CA, Andres CJ. The effect of tooth preparation design on the breaking strength of Dicor crowns: 3. *Int J Prosthodont* 1990; 3(4): 327-40. [PMID: 2088368]
- [9] Friedlander LD, Munoz CA, Goodacre CJ, Doyle MG, Moore BK. The effect of tooth preparation design on the breaking strength of Dicor crowns: Part 1. *Int J Prosthodont* 1990; 3(2): 159-68. [PMID: 2133383]
- [10] Burke FJ. Fracture resistance of teeth restored with dentin-bonded crowns: the effect of increased tooth preparation. *Quintessence Int* 1996; 27(2): 115-21. [PMID: 9063222]
- [11] McCormick JT, Rowland W, Shillingburg HTJ Jr, Duncanson MGJ Jr. Effect of luting media on the compressive strengths of two types of all-ceramic crown. *Quintessence Int* 1993; 24(6): 405-8. [PMID: 8234646]
- [12] Tuntiprawon M, Wilson PR. The effect of cement thickness on the fracture strength of all-ceramic crowns. *Aust Dent J* 1995; 40(1): 17-21. [http://dx.doi.org/10.1111/j.1834-7819.1995.tb05607.x] [PMID: 7710410]
- [13] Scherrer SS, de Rijk WG, Belser UC, Meyer JM. Effect of cement film thickness on the fracture resistance of a machinable glass-ceramic. *Dent Mater* 1994; 10(3): 172-7. [http://dx.doi.org/10.1016/0109-5641(94)90028-0] [PMID: 7758860]
- [14] Prakki A, Cilli R, Da Costa AU, Goncalves SE, Mondelli RF, Pereira JC. Effect of resin luting film thickness on fracture resistance of a ceramic cemented to dentin. *J Prosthodont* 2007; 16(3): 172-8. [http://dx.doi.org/10.1111/j.1532-849X.2006.00168.x] [PMID: 17581178]
- [15] Rojpaibool T, Leevailoj C. Fracture resistance of lithium disilicate ceramics bonded to enamel or dentin using different resin cement types and film thicknesses. *J Prosthodont* 2017; 26(2): 141-9. [http://dx.doi.org/10.1111/jopr.12372] [PMID: 26505488]
- [16] May LG, Kelly JR, Bottino MA, Hill T. Effects of cement thickness and bonding on the failure loads of CAD/CAM ceramic crowns: multi-physics FEA modeling and monotonic testing. *Dent Mater* 2012; 28(8): e99-e109. [http://dx.doi.org/10.1016/j.dental.2012.04.033] [PMID: 22595741]
- [17] Sagsöz NP, Yanıkoglu N, Yanıkoglu N. Evaluation of the fracture resistance of computer-aided design/computer-aided manufacturing monolithic crowns prepared in different cement thicknesses. *Niger J Clin Pract* 2018; 21(4): 417-22. [PMID: 29607851]
- [18] Hoang LN, Thompson GA, Cho SH, Berzins DW, Ahn KW. Die spacer thickness reproduction for central incisor crown fabrication with combined computer-aided design and 3D printing technology: An *in vitro* study. *J Prosthet Dent* 2015; 113(5): 398-404. [http://dx.doi.org/10.1016/j.prosdent.2014.11.004] [PMID: 25794915]
- [19] Paul F, Erdfelder E, Lang AG, Buchner AG. Power 3: A flexible statistical power analysis program for the social, behavioral, and biomedical sciences. *Behavior Research Methods Psychonomic Society Inc* 2007; 175-91. [http://dx.doi.org/10.3758/BF03193146]
- [20] Zahran M, El-Mowafy O, Tam L, Watson PA, Finer Y. Fracture strength and fatigue resistance of all-ceramic molar crowns manufactured with CAD/CAM technology. *J Prosthodont* 2008; 17(5): 370-7. [http://dx.doi.org/10.1111/j.1532-849X.2008.00305.x] [PMID: 18355164]
- [21] Neiva G, Yaman P, Dennison JB, Razzoog ME, Lang BR. Resistance to fracture of three all-ceramic systems. *J Esthet Dent* 1998; 10(2): 60-6. [http://dx.doi.org/10.1111/j.1708-8240.1998.tb00339.x] [PMID: 9759024]
- [22] Pallis K, Griggs JA, Woody RD, Guillen GE, Miller AW. Fracture resistance of three all-ceramic restorative systems for posterior applications. *J Prosthet Dent* 2004; 91(6): 561-9. [http://dx.doi.org/10.1016/j.prosdent.2004.03.001] [PMID: 15211299]
- [23] Kelly JR. Clinically relevant approach to failure testing of all-ceramic restorations. *J Prosthet Dent* 1999; 81(6): 652-61. [http://dx.doi.org/10.1016/S0022-3913(99)70103-4] [PMID: 10347352]
- [24] Lawn B. *Fracture of Brittle Solids*. 2nd ed. Cambridge, U.K.: Cambridge University Press 1993. [http://dx.doi.org/10.1017/CBO9780511623127]
- [25] Kelly JR. Dental ceramics: current thinking and trends. *Dent Clin North Am* 2004; 48(2): viii-, 513-530. [PMID: 15172614]
- [26] Attia A, Kern M. Fracture strength of all-ceramic crowns luted using two bonding methods. *J Prosthet Dent* 2004; 91(3): 247-52. [http://dx.doi.org/10.1016/j.prosdent.2003.12.005] [PMID: 15060494]
- [27] Attia A, Abdelaziz KM, Freitag S, Kern M. Fracture load of composite resin and feldspathic all-ceramic CAD/CAM crowns. *J Prosthet Dent* 2006; 95(2): 117-23. [http://dx.doi.org/10.1016/j.prosdent.2005.11.014] [PMID: 16473085]
- [28] Lampe K, Luthy H, Mörmann W. Fracture load of all-ceramic computer crowns. In: Mörmann W, Ed. *CAD/CIM in aesthetic dentistry: CEREC 10 Year Anniversary Symposium*. Chicago: Quintessence Pub 1996; pp. 463-82.
- [29] Kelly JR, Giordano R, Poher R, Cima MJ. Fracture surface analysis of dental ceramics: Clinically failed restorations. *Int J Prosthodont* 1990; 3(5): 430-40. [PMID: 2088380]
- [30] Zhao YF, Wang HR, Li Y. The effect of tooth preparation design on the CAD/CAM all-ceramic coping crown's fitness. *Zhonghua Kou Qiang Yi Xue Za Zhi* 2003; 38(5): 330-2. [PMID: 14680576]
- [31] Bindl A, Mörmann WH. Marginal and internal fit of all-ceramic CAD/CAM crown-copings on chamfer preparations. *J Oral Rehabil* 2005; 32(6): 441-7. [http://dx.doi.org/10.1111/j.1365-2842.2005.01446.x] [PMID: 15899023]
- [32] Prudente MS, Davi LR, Nabbout KO, *et al*. Influence of scanner,

- powder application, and adjustments on CAD-CAM crown misfit. *J Prosthet Dent* 2018; 119(3): 377-83.
[<http://dx.doi.org/10.1016/j.prosdent.2017.03.024>] [PMID: 28689912]
- [33] Zimmermann M, Valcanaia A, Neiva G, Mehl A, Fasbinder D. Digital evaluation of the fit of zirconia-reinforced lithium silicate crowns with a new three-dimensional approach. *Quintessence Int* 2018; 49(1): 9-15. [PMID: 29192293]
- [34] Kim J-H, Cho B-H, Lee J-H, *et al.* Influence of preparation design on fit and ceramic thickness of CEREC 3 partial ceramic crowns after cementation. *Acta Odontol Scand* 2015; 73(2): 107-13.
[<http://dx.doi.org/10.3109/00016357.2014.956145>] [PMID: 25299600]
- [35] Nakamura T, Dei N, Kojima T, Wakabayashi K. Marginal and internal fit of Cerec 3 CAD/CAM all-ceramic crowns. *Int J Prosthodont* 2003; 16(3): 244-8.
[PMID: 12854786]
- [36] Zeltner M, Sailer I, Mühlemann S, Özcan M, Hämmerle CHF, Benic GI. Randomized controlled within-subject evaluation of digital and conventional workflows for the fabrication of lithium disilicate single crowns. Part III: marginal and internal fit. *J Prosthet Dent* 2017; 117(3): 354-62.
[<http://dx.doi.org/10.1016/j.prosdent.2016.04.028>] [PMID: 27677220]
- [37] Mou SH, Chai T, Wang JS, Shiau YY. Influence of different convergence angles and tooth preparation heights on the internal adaptation of Cerec crowns. *J Prosthet Dent* 2002; 87(3): 248-55.
[<http://dx.doi.org/10.1067/mpr.2002.122011>] [PMID: 11941350]
- [38] Dauti R, Lilaj B, Heimel P, Moritz A, Schedle A, Cvikl B. Influence of two different cement space settings and three different cement types on the fit of polymer-infiltrated ceramic network material crowns manufactured using a complete digital workflow. *Clin Oral Investig* 2020; 24(6): 1929-38.
[<http://dx.doi.org/10.1007/s00784-019-03053-1>] [PMID: 31515700]
- [39] Kirsten M, Matta RE, Belli R, *et al.* Hygroscopic expansion of self-adhesive resin cements and the integrity of all-ceramic crowns. *Dent Mater* 2018; 34(8): 1102-11.
[<http://dx.doi.org/10.1016/j.dental.2018.04.008>] [PMID: 29709240]
- [40] Campagni WV, Preston JD, Reisbick MH. Measurement of paint-on die spacers used for casting relief. *J Prosthet Dent* 1982; 47(6): 606-11.
[[http://dx.doi.org/10.1016/0022-3913\(82\)90132-9](http://dx.doi.org/10.1016/0022-3913(82)90132-9)] [PMID: 7047724]
- [41] Hasanzade M, Shirani M, Afrashtehfar KI, Naseri P, Alikhasi M. *In vivo* and *in vitro* comparison of internal and marginal fit of digital and conventional impressions for full-coverage fixed restorations: A systematic review and meta-analysis *J Evid Based Dent Pract* 2019; 19(3): 236-54.
[<http://dx.doi.org/10.1016/j.jebdp.2019.04.003>] [PMID: 31732100]
- [42] Rekow ED, Harsono M, Janal M, Thompson VP, Zhang G. Factorial analysis of variables influencing stress in all-ceramic crowns. *Dent Mater* 2006; 22(2): 125-32.
[<http://dx.doi.org/10.1016/j.dental.2005.04.010>] [PMID: 16000218]
- [43] Pilo R, Cardash HS. *In vivo* retrospective study of cement thickness under crowns. *J Prosthet Dent* 1998; 79(6): 621-5.
[[http://dx.doi.org/10.1016/S0022-3913\(98\)70067-8](http://dx.doi.org/10.1016/S0022-3913(98)70067-8)] [PMID: 9627889]
- [44] Trindade FZ, Valandro LF, de Jager N, Bottino MA, Kleverlaan CJ. Elastic properties of lithium disilicate versus feldspathic inlays: Effect on the bonding by 3D finite element analysis. *J Prosthodont* 2018; 27(8): 741-7.
[<http://dx.doi.org/10.1111/jopr.12550>] [PMID: 27696615]
- [45] Charlton DG, Roberts HW, Tiba A. Measurement of select physical and mechanical properties of 3 machinable ceramic materials. *Quintessence Int* 2008; 39(7): 573-9.
[PMID: 19107265]
- [46] Bindl A, Lüthy H, Mörmann WH. Fracture load of CAD/CAM-generated slot-inlay FPDs. *Int J Prosthodont* 2003; 16(6): 653-60.
[PMID: 14714847]
- [47] Thompson JY, Bayne SC, Heymann HO. Mechanical properties of a new mica-based machinable glass ceramic for CAD/CAM restorations. *J Prosthet Dent* 1996; 76(6): 619-23.
[[http://dx.doi.org/10.1016/S0022-3913\(96\)90440-0](http://dx.doi.org/10.1016/S0022-3913(96)90440-0)] [PMID: 8957788]