


SUPPLEMENTARY MATERIAL

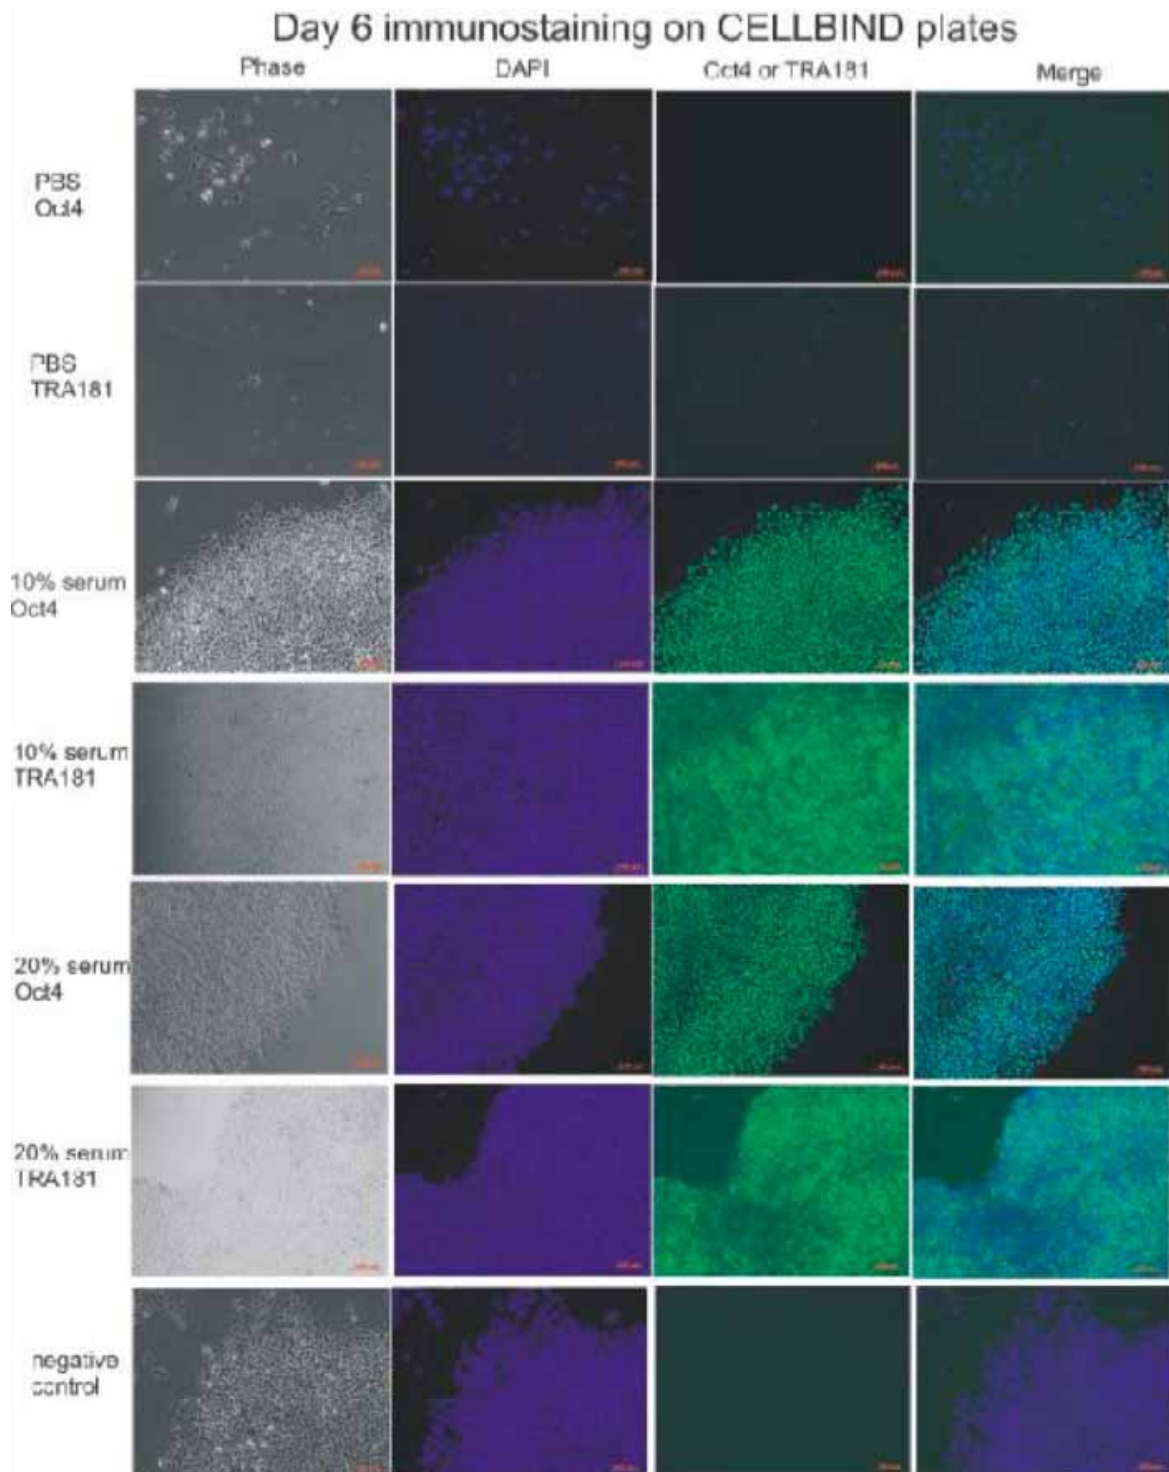

Supplemental Fig. (1). Immunostaining of Oct-4, TRA-1-81 and Hoechst-33342 on hESC-H1 maintained for 6 days in mTeSR1 on plastic dishes pre-coated with serum (10 and 20%) or without serum (PBS). Staining is indicated at the top part of each column, while the experimental conditions are indicated on the left side of each row. Left column: bright field, right column: merged images. Negative control for the antibodies are shown in the bottom row.